

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130306</u>
A	Name	<u>STEVE DUNN</u>	ID# <u>4106</u> Date <u>10-30-08</u>
	Agency	<u>APD</u>	Phone # <u>986-8900</u>
	Instrument Location	<u>SEELY SUB</u> ✓	
B	Alco S/N	<u>X172991</u>	Target Value <u>.077</u> High Pressure <u>400 PSI</u>
	Alco Test Value Average	<u>.074</u> ✓	<u>.073</u> ✓
		1 st Alco	2 nd Alco
Signature		<u>[Signature]</u> <u>CB</u> <u>11/20/08</u>	
(OVER)			


Under the Alaska Rules of Evidence, I certify that:
(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Steve P Dunn, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed

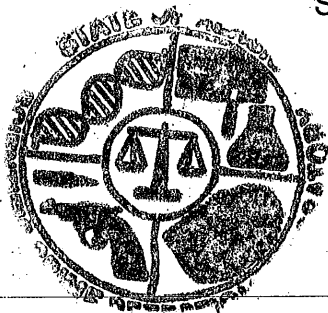

[Signature]

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

11/21/08
Date

NOV 03 2008

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130306 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

S. DUNN
#1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130306

OCTOBER 30, 2008 ✓

CD
11/20/08

OPERATOR'S NAME:

DUNN/S

OPERATOR'S NUMBER: 4106

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

U

O.L. #: U

DEPT/AGENCY: ANC1

CASE/REPORT: U

TEST TYPE: U

ALCO TARGET VALUE: .077 ✓

ALCO S/N: X172991

--- BREATH ANALYSIS ---

.077 ADJUSTED FOR 30.16 in		
ALCO TARGET	.077	14:49
BLANK TEST	.000	14:49
INTERNAL STANDARD	VERIFIED	14:50
ALCO TU 30.16 in	.074	14:50
BLANK TEST	.000	14:51
SUBJECT SAMPLE	.000	14:51
BLANK TEST	.000	14:52
ALCO TU 30.16 in	.073	14:53
BLANK TEST	.000	14:53

CD
11/20/08

DIAGNOSTIC CHECK

S. DUNN
#1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130306

OCTOBER 30, 2008 ✓

TIME 14:45

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	41c
BAROMETER:	30.16 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnopqrstuvwxyz{|}~